




Superior Biological Microscope, Quantum BM

Please read the User Manual carefully before using it and follow all operating and safety instructions!

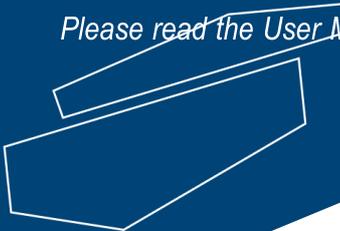

User Manual
English

User Manual



Superior Biological Microscope, Quantum BM

Preface

Users should read this Manual carefully, follow the instructions and procedures, and beware of all the cautions when using this instrument.

Service

If help is needed, you can always contact your dealer or Labbox via www.labbox.com (declare an incident). Please, provide the customer service representative with the following information:

- Serial number
- Description of the problem
- Your contact information

Warranty

This instrument is guaranteed to be free from defects in materials and workmanship under normal use and service, for a period of 24 months from the date of invoice. The warranty is extended only to the original purchaser. It shall not apply to any product or parts which have been damaged on account of improper installation, improper connections, misuse, accident or abnormal conditions of operation.

For claim under the warranty, please contact your supplier.

Contents

Before Use

1. COMPONENTS	1
2. ASSEMBLING	3
2-1 ASSEMBLING SCHEME	3
2-2 ASSEMBLING STEPS	4
3. OPERATION	6
3-1 SET ILLUMINATION	6
3-2 PLACE THE SPECIMEN SLIDE	6
3-3 ADJUST FOCUSING	6
3-4 ADJUST THE FOCUSING TENSION	7
3-5 ADJUST THE DIOPTR	7
3-6 ADJUST THE INTERPUPILLARY DISTANCE	7
3-7 ADJUST THE APERTURE DIAPHRAGM AND CONDENSER	8
3-8 USE THE OIL OBJECTIVE (100X)	8
3-9 USE THE COLOR FILTER	9
3-10 ASSEMBLE AND USE THE CTV DEVICE	9
4. TROUBLESHOOTING	10

Before Use

1. Operation Notice

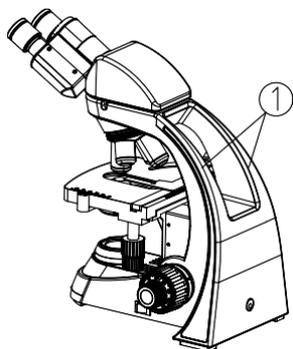


Fig.1

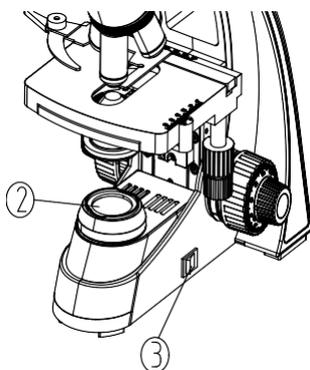


Fig.2

1. As the microscope is a high precision instrument, always operate it with care, and avoid physical shake during the operation.

2. Do not expose the microscope in the sun directly, either not in the high temperature, damp, dust or acute shake. Make sure the worktable is flat and horizontal. The following environment is required when operating:

Indoor temperature:
5°C ~ 40°C, Max relative humidity: 80%.

3. When moving the microscope, use both hands to hold its arm①, and lay it down carefully (see Fig. 1).

★ **It will damage the microscope by holding the stage, focusing knob or head when moving.**

4. When working, the surface of the condenser will be very hot. Make sure there is enough room for the heat dissipating around the condenser② (see Fig. 2).

5. For safety, make sure the power switch is at "O" (OFF) and power it off before replacing the bulb or fuse (See Fig. 2), and wait until both the bulb and bulb holder have cooled down.

6. Standard bulb: Single 3W LED bulb.

7. All the power OFF devices have been set in the position where is easy to operate.

8. No contraindications for this product.

2. Maintenance

1. Wipe the lens gently with a soft tissue. Carefully wipe off the oil marks and fingerprints on the lens surfaces with a tissue moistened with a small amount of 3:7 mixtures of alcohol and ether or dimethylbenzene.

★ As the alcohol and ether are flammable, don't place these chemicals near to fire or fire source. For example, when turning on or turning off the electrical device, please use these chemicals in a ventilated place.

2. Don't use organic solutions to wipe the surfaces of the other components. Please use the neutral detergent if necessary.

3. If the microscope is damped by liquid when using, please power it off immediately and wipe it dry.


4. Never disassemble the microscope, otherwise the performance will be affected, or the instrument will be damaged.


5. After using it, cover the microscope with a dust cover.

3. Safety Sign

Sign	Signification
	Study the instructions before use. Unsuitable operation would lead to a person being hurt or instrument faulty.
I	Main switch ON
O	Main switch OFF

1. Components

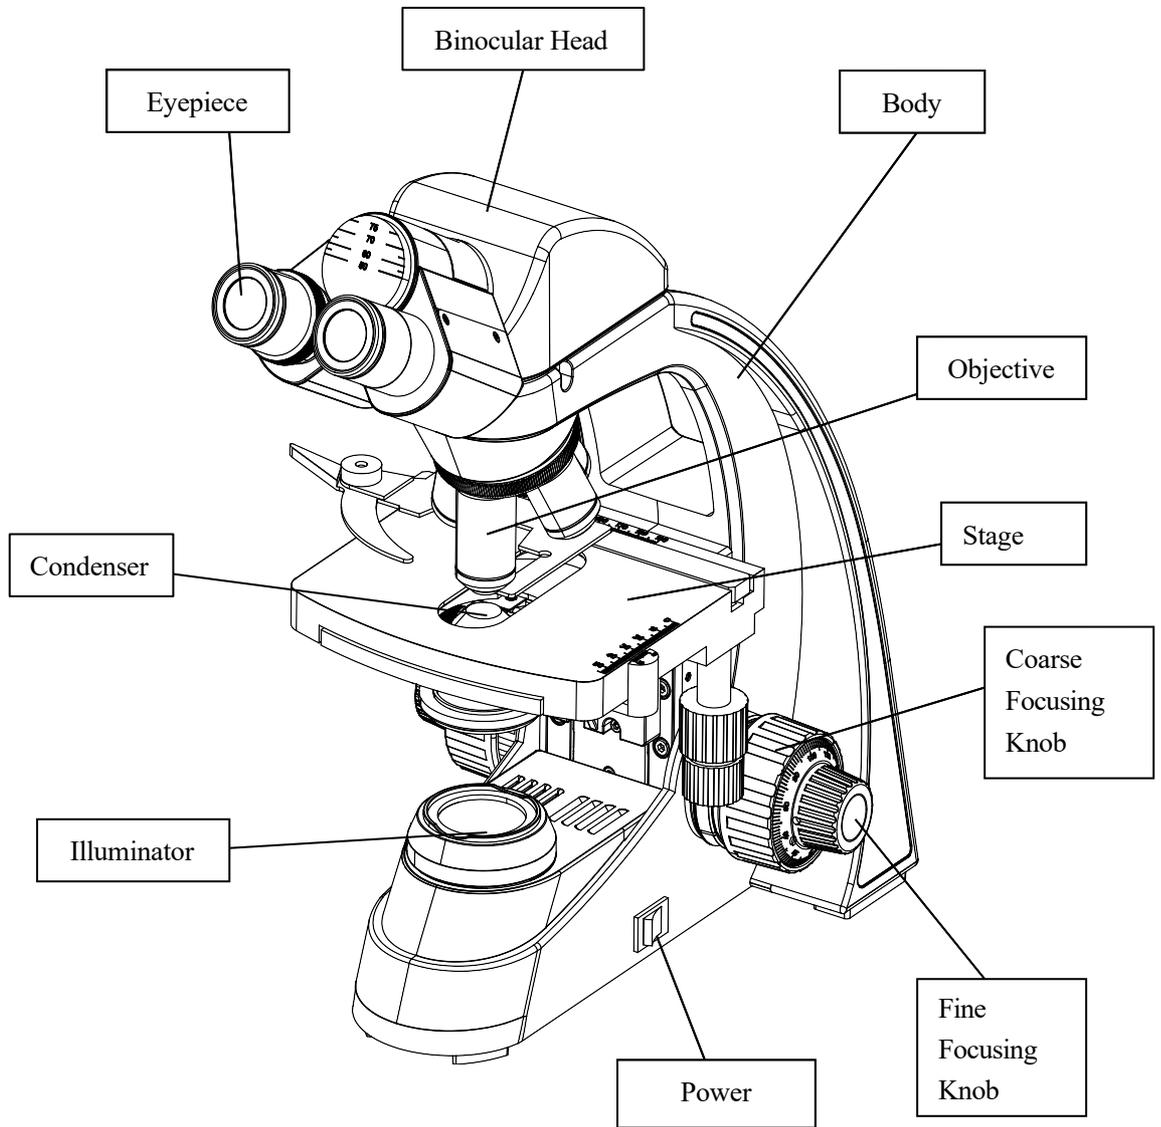

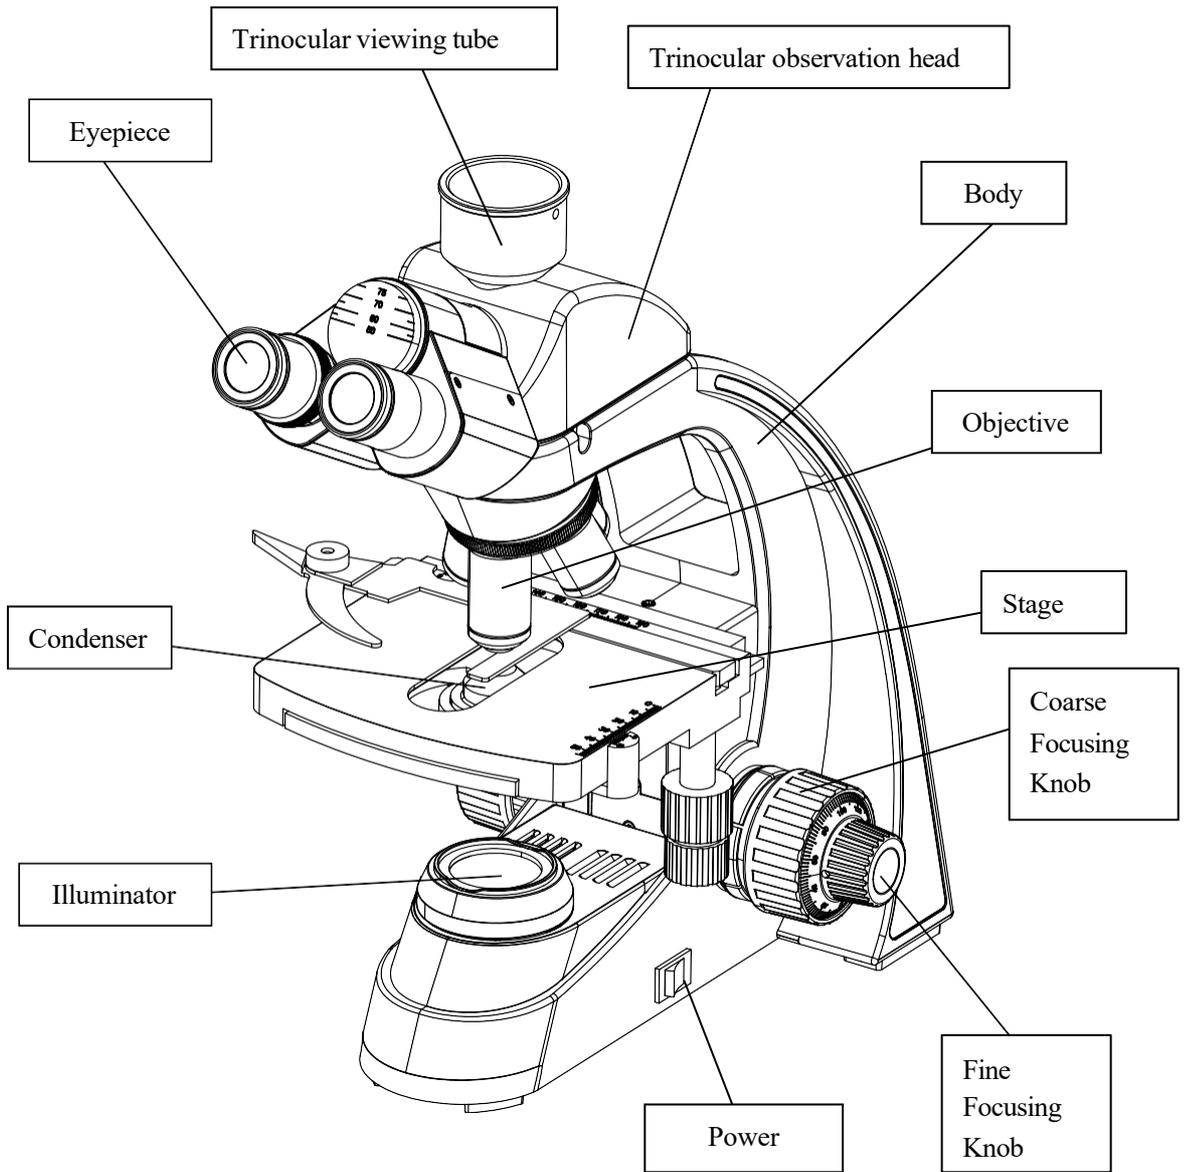


2. Assembling

2-1 Assembling Scheme

The following is the Assembling Scheme, and the numbers denote the assembling order.

★ Before assembling, make sure there is no dust or dirt. Assemble carefully and do not scrap any part or touch the glass surface.

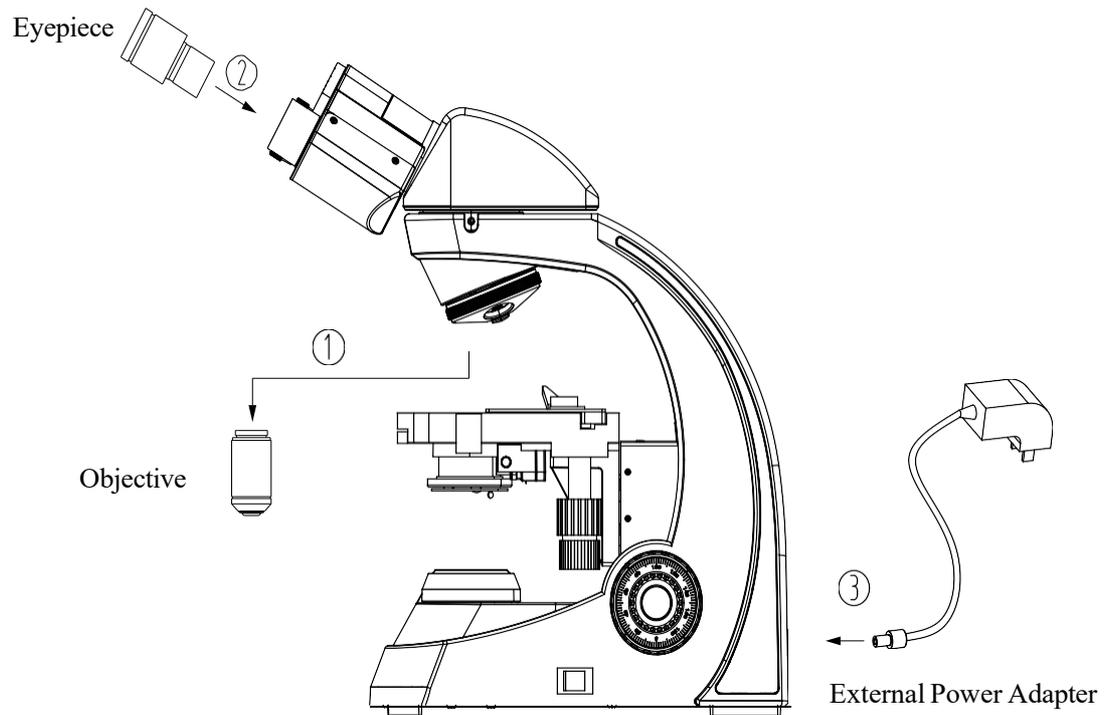

2-2 Assembling Steps

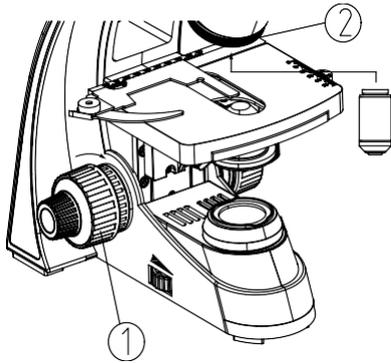


Fig.3

2-2-1 Assemble the Objective

1. Rotate the coarse focusing knob ① to lower the stage to a suitable location (See Fig.3).
2. Install the objectives into the nosepiece from the lowest magnification to the highest in a clockwise direction.

★ Search and focus the sample by low Magnification objective (4X or 10X) when operating. Then change to the high magnification ones according to the observation requirements.

★ When replacing the objective, rotate the nosepiece until it sounds “ka-da”, to make sure the objective is in the centre of the light path.

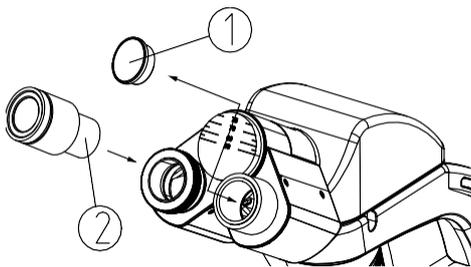


Fig.4

2-2-2 Assemble the Eyepiece

1. Take down the cover of eyepiece tube ①.
2. Insert the eyepiece ② into the eyepiece tube, until touch the bottom (See Fig. 4).

2-2-3 Assemble or replace the LED

Screw out the lock screw on the bottom group and take out the bottom group. Press on snaps on the connector socket ① (connected with LED control panel) according to the direction of the arrow as shown in the figure, pull out the connector ② (connected with LED). Then screw out the two screws ③ that fixed the LED, replace with a new LED group. Fix the LED group by the two screws, plug the connector ② into connector socket ①, assemble the bottom group to original place (See Fig.5).

★ Before replacing the LED, make sure to cut off the main power and wait for LED group to cool down, to avoid overheating and burning.

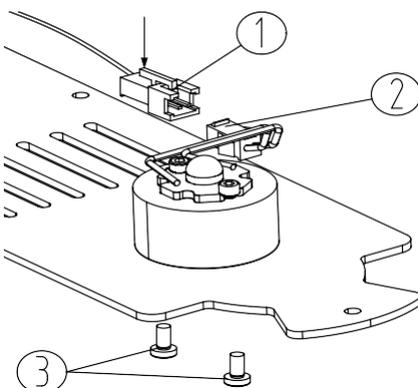


Fig.5

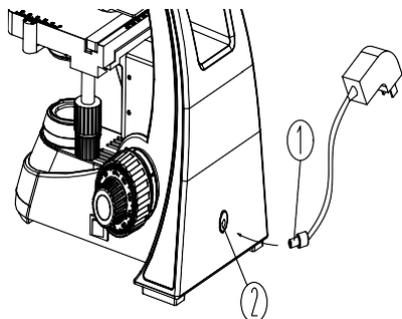


Fig.6

2-2-4 Connect the External Power Adapter (Power Cord/Charger)

- ★ Don't use strong force when the power cord is bent or twisted, otherwise it will be damaged.
- ★ Use the special external power adapter (power cord/charger) supplied by our company. If it's lost or damaged, choose one with the same specifications.

◎ For External Power Adapter

1. Make sure the power switch is at "O" (OFF).
2. Insert one end of external power adapter① into the power socket② of the microscope. Then insert the other end into the power supply socket and make sure well-connected (See Fig. 6).

- ★ Adopt DC6V 2A external power supply. Make sure to use an external power adapter complies with this requirement.
- ★ The models with rechargeable battery must use DC6V 1A external battery charger for charging. When the instrument is fully charged, the charger indicator will change from orange to green. When replacing rechargeable batteries, use high-quality 5 # rechargeable battery.

3. Operation

3-1 Set Illumination

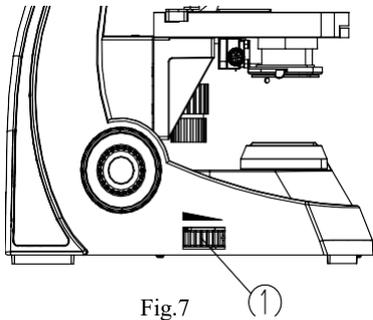


Fig.7

1. Put through the power and turn on the main power switch to “—” (ON).
2. Adjust the light adjustment knob ① until the illumination is comfortable for observation. Rotate the light adjustment knob clockwise to raise the voltage and brightness. Rotate the light adjustment knob counterclockwise to lower the voltage and brightness (see Fig. 7).

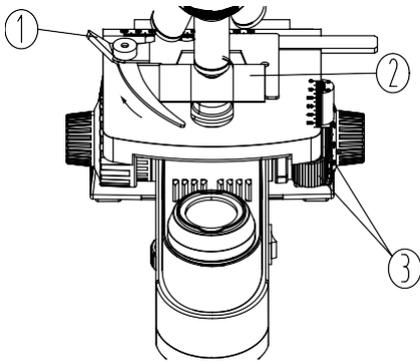


Fig.8

3-2 Place the Specimen Slide

1. Push the wrench of the specimen holder backwards.
2. Loosen the wrench ① and clamp the slide ② by the clips while the cover glass faces up (see Fig. 8).
3. Rotate the X and Y-axis knob ③. Move the specimen to the center (alignment with the center of the objective).

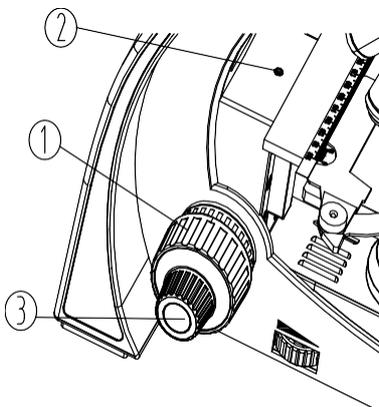


Fig.9

3-3 Adjust Focusing

1. Shift the 4X objective into the light path.
 2. Observe the right eyepiece with the right eye. Rotate the coarse focusing knob ① until the image outline appears in the view field (See Fig.9).
 3. Rotate the fine focusing knob ③ for clear details.
- ★ The lock screw ② can prevent the objective touching the slice when focusing.

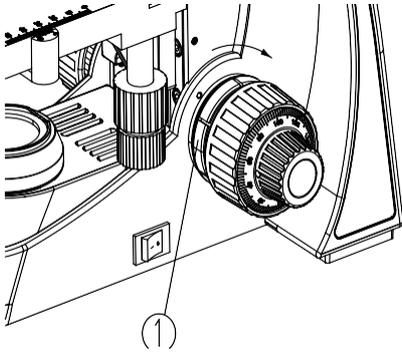


Fig.10

3-4 Adjust the Focusing Tension

If the handle is very heavy when focusing or the specimen leaves the focus plane after focusing, or the stage declines itself, rotate the tension adjustment knob ① to resolve the problem (See Fig. 10).

Rotate the tension adjustment knob ① according to the direction of the arrow as shown in the figure, to lock the focusing system. Rotate it to the opposite direction to loosen the focusing system.

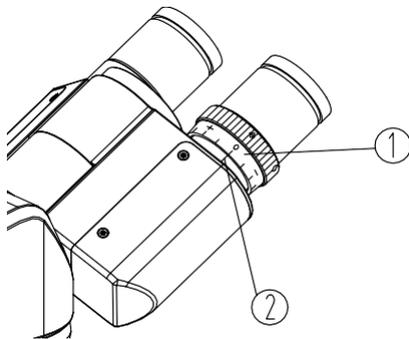


Fig.11

3-5 Adjust the Dioptre

Observe the right eyepiece with the right eye, focus it until the image is clear. Then observe the left eyepiece with the left eye, if the image is not clear enough, rotate the dioptre adjustment ring ① until the image is clear (See Fig.11).

★ There are ± 5 dioptres on the dioptre adjustment ring ①, and the value aligned with the scale ② is your eye's dioptre.

★ When using dioptre adjustable eyepiece, do eyepiece dioptre zero adjustment first. Adjust eyepiece dioptre to make the image clear when operating.

★ Remember your eye's dioptre, so that you can use it next time.

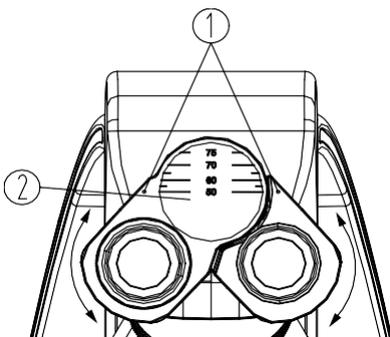


Fig.12

3-6 Adjust the Inter-pupillary Distance

When using two eyes to observe, hold the bases of the prism and rotate them around the axis to adjust the inter-pupillary distance, until there is only one field of view. The dot “.” ① on the eyepiece base points to the scale ② of the inter-pupillary distance indicator. The scale value is the inter-pupillary distance (See Fig. 12).

Adjustable range: 50~75mm.

★ Remember your eye's inter-pupillary distance, so that you can use it next time.

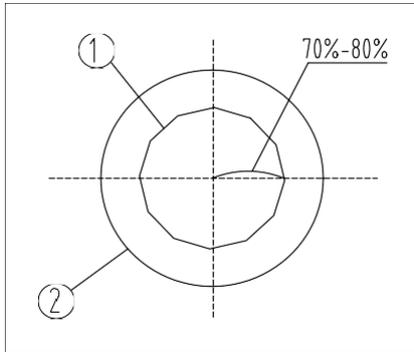


Fig.13

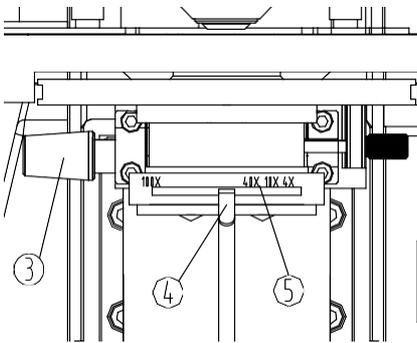


Fig.14

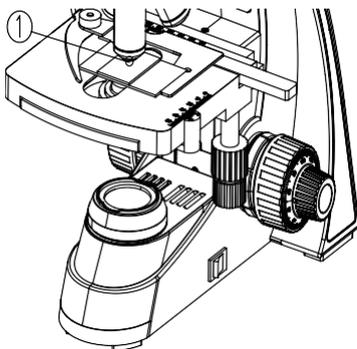


Fig.15

3-7 Adjust the Aperture Diaphragm and Condenser

1. The aperture diaphragm decides the numerical aperture of the illumination system. If the N.A. illumination system matches with the N.A. of the objective, it can obtain better resolution and contrast and increase the depth of field.

2. Adjust condenser adjustment knob③ in clockwise direction, raise the condenser to the top, let the illumination light fill the field of view. As the specimen contrast is usually low, it is advised to adjust the condenser aperture diaphragm to be 70%-80% of the N.A. of objective. Rotate the aperture diaphragm adjusting ring④, align the arrow with the magnification position on the diaphragm seat⑤. The eyepiece can be taken off when it's necessary to observe from the tube. Adjust the aperture diaphragm adjusting ring④ until see the figure as shown in Fig. 13, to adjust the proportion (see Fig. 13&14, ① is the image of aperture diaphragm, ② is the edge of objective).

3-8 Use the Oil Objective (100X)

1. Use the 4X objective to focus the specimen.
2. Place a drop of oil① on the specimen (see Fig. 15).
3. Rotate the nosepiece counterclockwise and rotate the oil objective (100X) to the light path. Then use the fine focusing knob to focus.

★ **Make sure there is no air bubble in the oil for fear affect the image.**

A. Move the eyepiece to examine the air bubble. Open the aperture diaphragm and field diaphragm fully and observe the edge of the objective from the tube (It seems round and light).

B. Rotate the nosepiece slightly and swing the oil objective for some times to remove the air bubble.

4. After using, wipe the front lens with a tissue moistened with a small amount of 3:7 mixture of alcohol and ether or with dimethylbenzene. Wipe off the oil on the specimen.

★ **Don't put another objective to the light path before the oil is wiped to avoid wetting the dry objective.**

★ **Too much dimethylbenzene would dissolve the lens's stickiness.**

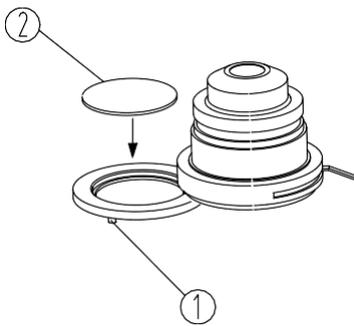



Fig.16

3-9 Use the Colour Filter

Screw out the colour filter frame ① at the bottom of the condenser in clockwise direction, press the filter ② into its hole, then screw in the frame in counterclockwise direction (See Fig.16).

★ **There are three colours of filter selectable: blue, green and yellow.**

3-10 Assemble and use the CTV Device

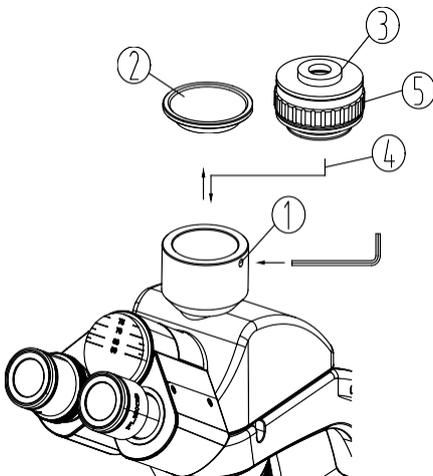

1. Loosen the lock screw ① of trinocular head and take out the dustcover ② (See Fig.21).

2. Take down the dustcover of the CTV adapter ③. Insert the CTV adapter into the trinocular head as shown in the figure and screw down the lock screw ①.

3. Loosen the lock screw ④ of the CTV adapter. Take down the vidicon interface (C type) ⑤ from the CTV adapter, and screw into the CCD or vidicon.

Then install the interface into the CTV adapter, and screw down the lock screw ④.

4. For binocular observation, observe CCD image when the image is clear. If the image is unclear, rotate the adjustment tube ⑥ until it is clear.

4. Troubleshooting

As the performance of microscope can't play fully due to unfamiliar operations, the table below can provide some solutions.

Problem	Cause	Solution
1. Optical system		
(1) The bulb is bright, but it is dark in the field of view.	Field diaphragm is not large enough.	Enlarge the field diaphragm.
	The condenser is too low.	Adjust the condenser.
(2) The side of the field of view is dark or not even.	Nosepiece is not in the right position.	Turn the nosepiece into the right position.
	Stain or dust has accumulated on the lens (condenser, objective or eyepieces).	Clean the lens.
(3) Stain or dust is observed in the field of view.	Stains have accumulated on the specimen.	Clean the specimen.
	Stains have accumulated on the lens.	Clean the lens.
(4) Unclear image	No cover glass on the specimen slide.	Add the cover glass.
	The cover glass is not standard.	Use a standard cover glass with thickness of $\delta 0.17\text{mm}$.
	The specimen faces down.	Put the specimen to face up.
	The immersion oil has accumulated on the dry objective.	Clean thoroughly.
	The immersion oil is not used for oil objective.	Use immersion oil.
	Air bubble in the immersion.	Get rid of the air bubble.
	Use wrong immersion oil.	Use a correct one. (Cedar oil)
	The aperture diaphragm is not opened correctly.	Adjust it.
	Stain or dust has accumulated on the lens of eyepiece.	Clean the lens.
	The condenser is too low.	Adjust the condenser.
(5) One side of the image is dark, or the image moves while focusing.	The specimen slide is not fixed.	Fix it with clips.
	Nosepiece is not in the right position.	Turn the nosepiece into the right position.
	The condenser is not centred.	Centre the condenser.
(6) The eyes feel tired easily. The right field of view doesn't superpose with the left.	Interpupillary distance is incorrect.	Adjust the interpupillary distance.
	The eyepiece for the right eye is different from the left one.	Use the same eyepieces.

Problem	Cause	Solution
2. Mechanical system		
(1) Cannot focus when using high magnification objective.	The cover glass faces down.	Put the cover glass to face up.
	The cover glass is too thick.	Use a standard cover glass with thickness δ 0.17mm.
(2) The objective touches the cover glass while turning the nosepiece.	The cover glass faces down.	Put the cover glass to face up.
	The cover glass is too thick.	Use a standard cover glass with thickness δ 0.17mm.
(3) Coarse focusing knob is too tight.	The tension adjustment knob is too tight.	Loosen it to an appropriate position.
(4) Stage declines itself and cannot stay on the focal plane.	The tension adjustment knob is too loose.	Tighten it to an appropriate position.
(5) Coarse focusing knob cannot rise.	The coarse focusing limit knob is locked.	Loosen the coarse focusing limit knob.
(6) Coarse focusing knob can't decline.	The base of the condenser is too low.	Raise the base.
(7) Cannot move the slide smoothly.	The slide is not fixed correctly.	Adjust it correctly.
	The movable specimen holder is not fixed properly.	Adjust it correctly.
(8) The image moves obviously when touching the stage.	The stage is fastened incorrectly.	Fasten the stage correctly.
3. Electrical Part		
(1) The bulb does not work.	No power supply.	Check the connection of the power cable.
	The bulb is not installed correctly.	Install it correctly.
	The bulb burns out.	Replace it.
(2) The bulb burnt out usually	A wrong bulb is used.	Replace it with a correct one.
(3) The field of view is not bright enough	A wrong bulb is used.	Replace it with a correct one.
	The use of light adjusting knob is incorrect.	Adjust it correctly.

Nota importante para los aparatos electrónicos vendidos en España

Instrucciones sobre la protección del medio ambiente y la eliminación de aparatos electrónicos:



Los aparatos eléctricos y electrónicos marcados con este símbolo no pueden ser eliminados en forma de residuos urbanos.

De conformidad con la Directiva 2012/19/UE, los usuarios de la Unión Europea de aparatos eléctricos y electrónicos, tienen la posibilidad de devolver sus RAEE para su eliminación al distribuidor o fabricante del equipo después de la compra de uno nuevo. La eliminación ilegal de aparatos eléctricos y electrónicos es castigada con multa administrativa.

Remarque importante pour les appareils électroniques vendus en France

Informations sur la protection du milieu environnemental et élimination des déchets électroniques :



Les appareils électriques et électroniques portant ce symbole ne peuvent pas être jetés dans les décharges.

En réponse à la réglementation, Labbox remplit ses obligations relatives à la fin de vie des équipements électriques de laboratoire qu'il met sur le marché en finançant la filière de recyclage de ecosystem dédiée aux DEEE Pro qui les reprend gratuitement (plus d'informations sur www.ecosystem.eco).

L'élimination illégale d'appareils électriques et électroniques est punie d'amende administrative.

Nota importante per le apparecchiature elettroniche vendute in Italia

Istruzioni sulla protezione ambientale e sullo smaltimento dei dispositivi elettronici:



Le apparecchiature elettriche ed elettroniche contrassegnate con questo simbolo non possono essere smaltite come rifiuti urbani.

In conformità con la Direttiva 2012/19 / UE, gli utenti dell'Unione Europea di apparecchiature elettriche ed elettroniche hanno la possibilità di restituire i propri RAEE per lo smaltimento al distributore o al produttore di apparecchiature dopo averne acquistato uno nuovo. La rimozione illegale di apparecchiature elettriche ed elettroniche è punibile con una sanzione amministrativa.

www.labbox.com